



The impact of physiological and parafunctional posterior occlusal forces on experimental Ti-15Zr supracrestal dental implant – a finite element analysis

Brigitta Bokor¹, Adriana Objelean², Simion Bran³, Radu Septimiu Campian⁴, Cristian Vilău⁵

1) Doctoral School, Department of Oral Rehabilitation, Faculty of Dentistry, Iuliu Hatieganu University of Medicine and Pharmacy, Cluj-Napoca, Romania

2) Department of Prosthetics and Dental Materials, Faculty of Dentistry, Iuliu Hatieganu University of Medicine and Pharmacy, Cluj-Napoca, Romania

3) Department of Maxillofacial Surgery and Implantology, Faculty of Dentistry, Iuliu Hatieganu University of Medicine and Pharmacy, Cluj-Napoca, Romania

4) Department of Oral Rehabilitation, Faculty of Dentistry, Iuliu Hatieganu University of Medicine and Pharmacy, Cluj-Napoca, Romania

5) Department of Material Resistance, Faculty of Mechanical Engineering, Technical University of Cluj-Napoca, Romania

Abstract

Aim of the study. This study aims to evaluate and compare the stress distribution patterns of two experimental tissue-level, convergent collar implants (one made of Ti-6Al-4V (control) and the other of Roxolid-based (Ti-15Zr) material) using 3D finite element analysis (FEA) under various simulated masticatory conditions.

Methods. A 3D finite element model replicating a tissue-level implant with convergent neck design was developed in ANSYS software, incorporating both cortical and trabecular bone geometry. Implants made of Ti-6Al-4V-Grade 5 and Roxolide-type-Ti-15Zr alloy were simulated under axial (0°) and oblique (45° angle) loading forces (50 N, 200 N, 300 N, and 400 N). The von Mises equivalent stress distribution was calculated to assess the biomechanical performance.

Results. Under masticatory forces simulation, titanium-alloy implants exhibited maximum stress values (400 N) of 260.38 MPa under axial load and 536.2 MPa under oblique load. Ti-15Zr implants exhibited a slightly lower peak stress of 506.95 MPa under a load of 400 N at a 45° inclination and 240.81 N under axial load. Based on 3D finite analysis, the stress distribution maps showed higher concentration in the implant–abutment connection and the cervical region, particularly under oblique loading.

Conclusions. Although titanium implants exhibited higher stress limits, Ti-15Zr implants showed biomechanical stability under oblique simulated forces. Ti-15Zr implants exhibited a more uniform stress distribution with a reduced peak concentration.

Keywords: finite element analysis, Ti-15Zr implants, titanium implants, Roxolid, supracrestal implant, parafunctional forces, tissue-level implant, convergent collar

DOI: 10.15386/mpr-2930

Manuscript received: 30.05.2025

Received in revised form: 24.08.2025

Accepted: 10.09.2025

Address for correspondence:

Adriana Objelean

adriana.caracostea@elearn.umfcluj.ro

This work is licensed under a Creative Commons Attribution-NonCommercial-NoDerivatives 4.0 International License <https://creativecommons.org/licenses/by-nc-nd/4.0/>

Introduction

Edentulism is a medical condition affecting patients in multiple ways, including aesthetics, mental health, and overall wellness. As a result, dental professionals utilize various treatment options, including fixed partial dentures, removable prostheses, and dental implants [1-7]. However, to overcome the limitations of both fixed and removable partial dentures and to protect the mucosal tissues and alveolar

ridge, dental implants are increasingly recommended [1-7].

For the past sixty years, dental implants have been established as the gold standard in prosthetic dentistry, offering patients with partial or complete tooth loss predictable, long-term results [3]. The success of implants relies on two main pillars: osseointegration and mechanical stability. Titanium and its alloys, particularly Ti-6Al-4V, have led the field due to their excellent fatigue and

corrosion resistance, and also proven biocompatibility, which has been demonstrated over many years of clinical use [2,3,5]. However, attention has increased because of some limitations of titanium-based implants, including aesthetic issues for patients with thin gum tissue, their potential to corrode in saliva and fluoride environments, and growing concerns about titanium particle-induced inflammation and peri-implantitis [8-10].

Under the clinical conditions mentioned above, there is a high demand for metal-free and aesthetically superior options, leading researchers and clinicians to develop and use Roxolid (Ti-15Zr), zirconium-based and ceramic-based implants in clinical settings [11-16]. Roxolid-type implants (Ti-15Zr) are currently the most extensively studied ceramic-based implant materials. Roxolid (Ti-15Zr) provides high flexural strength, resistance to crack growth, chemical inertness, and a tooth-like white color, making it suitable for use in highly aesthetic areas [11,12,14,15]. Additionally, *in vitro* and *in vivo* studies have demonstrated that Roxolid (Ti-15Zr) implants exhibit less bacterial colonization and biofilm formation compared to titanium, potentially reducing the risk of peri-implant inflammation and mucositis [9-12]. Moreover, histological evaluations in animal models have demonstrated similar bone-to-implant contact (BIC) for both titanium and Roxolid type (Ti-15Zr) surfaces when proper surface treatments - such as sandblasting and acid-etching. However, concerns about the material's brittle nature, susceptibility to low-temperature degradation (tetragonal-to-monoclinic phase change), and limited long-term survival data remain significant in clinical practice [17-21].

The oral cavity subjects implant-based dental materials to withstand its hostile conditions. One of these conditions is the occlusal status; for instance, this may involve initial parafunctional chewing forces (e.g., clenching teeth, bruxism, etc) when the teeth are present, and these continue even after the teeth are extracted. Moreover, it is known that these high occlusal forces have increased values in the posterior zone compared with the rest of the areas [22-27]. Thus, it is essential to evaluate and consider this when dental titanium or titanium-zirconium-based implants are indicated for missing teeth in the lateral zone.

Different *in vitro* experiments and test simulations were imagined, but the new digital testing simulation techniques, such as three-dimensional finite element analysis (3D-FEA) assessments, have gained popularity to be used to identify more easily the stress distribution and occlusal stress for various dental biomaterials [24,25,27,28].

Reports of FEA tests have consistently shown that Roxolid-based (Ti-15Zr) implants accumulate higher peak von Mises stresses, particularly at the implant neck and crestal bone, when subjected to oblique forces above 300

N [13,14]. This stress localization significantly increases the risk of mechanical failure in posterior regions.

Different systematic reviews or meta-analyses of clinical reports have corroborated these findings, highlighting higher fracture rates for two-piece implants under occlusal stress, as well as technical complications during insertion due to the material's low ductility [14-17,28,29]. However, based on our search, the suitability of supracrestal Ti-Grade 5 and Roxolid-based (Ti-15Zr) implants subjected to parafunctional masticatory forces has not been widely tested.

This study aims to assess the stress distribution patterns of two experimental tissue-level, convergent collar implants—one made of titanium Grade 5 (Ti-6Al-4V alloy) and the other of Roxolid-based (Ti-15Zr) material—simulated during a clinical setup scenario with standardized axial and oblique parafunctional masticatory forces using 3D finite element analysis (FEA). We formulated the following hypotheses: H1) The Ti-15Zr-based dental implant will exhibit higher von Mises stress limits than the Ti-6Al-4V implant; H2) The Roxolid-type Ti-15Zr-based dental implant will demonstrate uneven mechanical behavior under oblique simulated parafunctional chewing forces.

Methods

Implant design and 3D modelling

For this experimental study, we combined the geometry of a newly developed commercial implant system (tissue-level supracrestal implant, Prama Power Regular Neck implant, Sweden&Martina, Padua, Italy) and two types of dental implant alloys (Ti-4Al-6V alloy (control) and Roxolid-type Ti-15Zr alloy (Roxolid, Institut Straumann AG)).

The features of the implants used in this study were based on the anatomy of a first mandibular molar and on the geometry of the previously mentioned commercially available supracrestal implant systems, which incorporate a transmucosal collar modeled as a smooth neck of 2.8 mm high, mimicking the emergence profile commonly used in soft tissue-friendly implant designs, to promote soft tissue stability and biological sealing [30].

The implant was designed as a cylindrical, tissue-level body with a convergent neck measuring 3.8 mm in diameter and 11.5 mm in length, featuring thread geometry at both the apical and crestal regions.

Tissue-level implant designs are extensively recognized in clinical practice for their capacity to reduce bacterial microleakage and to diminish crestal bone remodeling by positioning the implant-abutment interface away from the alveolar crest. Additionally, their design helps preserve peri-implant soft tissue integrity throughout both prosthetic and surgical phases, thereby minimizing inflammation and promoting long-term peri-implant health [30].

All the aforementioned characteristics were applied in both Ti-6Al-4V and Roxolid-type (Ti-15Zr) models for biomechanical consistency.

Figure 1 illustrates the implant placement within a bone block that simulates the mandibular ridge, characterized by a cortical outer layer and a trabecular core. The implant replicates a tissue-level implant design featuring a transmucosal collar.

A CAD model was utilized for the implant design. The implant features a standard cylindrical thread geometry, an internal hexagonal connection, and an apically tapered end. The design reflects real-life tissue-level implant systems used in clinical settings (Figure 2).

Meshing strategy

The implant-bone assembly was discretized using a finite element mesh composed of tetrahedral elements. A global mesh size of 0.5 mm was adopted to balance computational efficiency with solution accuracy, particularly in the vicinity of the implant threads and cortical interface, where stress concentration was expected (Figure 3).

Mesh sensitivity tests compared finer (0.25 mm) meshes with the 0.5 mm mesh to verify that the von Mises stress (vM) values are within a 5% error margin, confirming their consistency.

Material properties assignment

All materials were assumed to be homogeneous, isotropic, and linearly elastic. Additionally, for the Stability factor, the bone and the dental implants were considered to undergo complete osseointegration.

Mechanical properties

Regarding material selection for dental implantology, titanium alloy is one of the most often used and tested materials [2-4]. For this experimental study, the following dental implant materials were considered: a Ti-6Al-4V alloy (control) and Roxolid-type alloy (Ti-15Zr). For both types of materials, a tissue-level convergent neck implant design was designed. The mechanical properties were assigned based on values reported in the literature (Table I) [31-36].

Geometry

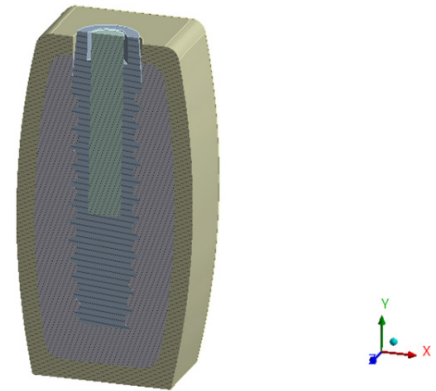


Figure 1. Cross-sectional 3D geometry of the finite element model used in the study.

Geometry

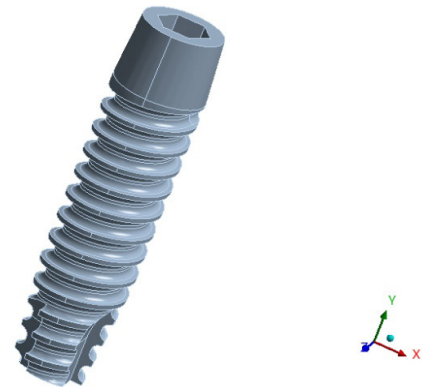


Figure 2. The CAD model used for the supracrestal with convergent neck Ti-Grade 4/Ti-15Zr implants was analyzed using 3D finite element analysis.

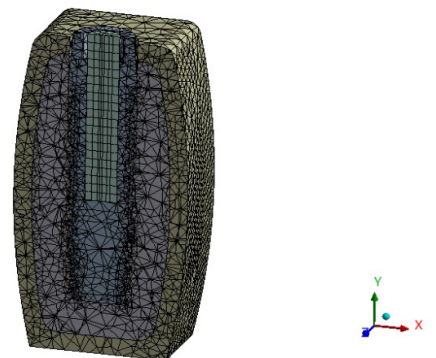


Figure 3. Meshing system used in the study.

Table I. Mechanical properties [31-36].

Component	Material	Young's Modulus (GPa)	Poisson's Ratio
Implant 1	Ti-6Al-4V	110	0.34
Implant 2	Ti-15Zr	103.7	0.33
Cortical Bone	Human Cortical Bone	14.7	0.30
Trabecular (spongy, cancellous) Bone	Human Trabecular Bone	1.47	0.30

Boundary conditions and load application

All the surfaces of the bone block were fully constrained to simulate physiological fixation. No implant displacement was allowed at the apical or lateral walls of the bone.

Loading was applied axially (0°) and obliquely (45°) to the occlusal surface of the implant, simulating parafunctional masticatory forces. The magnitude of force was incrementally increased: 50 N, 100 N, 200 N, 300 N, and 400 N.

Figure 4 illustrates the two loading scenarios employed as a simulation setup for the physiological and parafunctional occlusal forces:

- Scenario A (physiological): Axial loading (0°) to simulate biting force on the posterior teeth.
- Scenario B (parafunctional): Oblique loading (45° angle) to simulate paraxial lateral chewing in the posterior zone.

Each scenario was applied independently to both Ti-6Al-4V and Roxolid-type (Ti-15Zr) tissue-level implants utilizing identical mesh and boundary conditions.

Stress evaluation and output analysis

The output of interest was the maximum von Mises stress values (vM), evaluated across the entire implant structure and at the implant-bone interface. ANSYS 2024R2 software (Ansys Workbench, Canonsburg, PA,

USA) was utilized for three-dimensional static analysis.

Solver parameters were configured for static structural analysis. Results were visualized using stress contour plots, and values were extracted at key-point regions: the implant shoulder, the first thread, and the cortical interface.

Representative stress distribution maps were captured directly from ANSYS and are shown in figure 5, figure 6, figure 7 and figure 8.

Results

The numerical analysis showed differences in von Mises (vM) stress distribution between Ti-based alloy and Roxolid-type (Ti-15Zr) tissue-level implants under variable loading conditions. As the applied force increased from 50 N to 400 N, and the angle of application changed from axial (0°) to oblique (45°), stress magnitudes rose consistently in both materials (Figure 9).

Under a 50 N axial load, the Ti-Grade 5 implant displayed a uniform and low-stress field, with peak values of approximately 32.5 MPa, primarily found in the first thread region and the cortical bone interface. Under the same loading conditions, the Ti-15Zr implant showed a slightly lower peak stress of 30.1 MPa, with a more localized concentration near the implant shoulder. As forces increased to 400 N axially, Ti-Grade 5 reached a maximum stress of approximately 260.38 MPa.

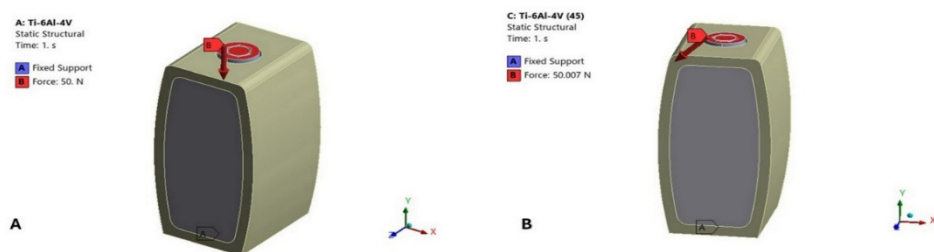


Figure 4. The loading simulated scenarios. A) axial loading (0°) and B) oblique loading (45°).

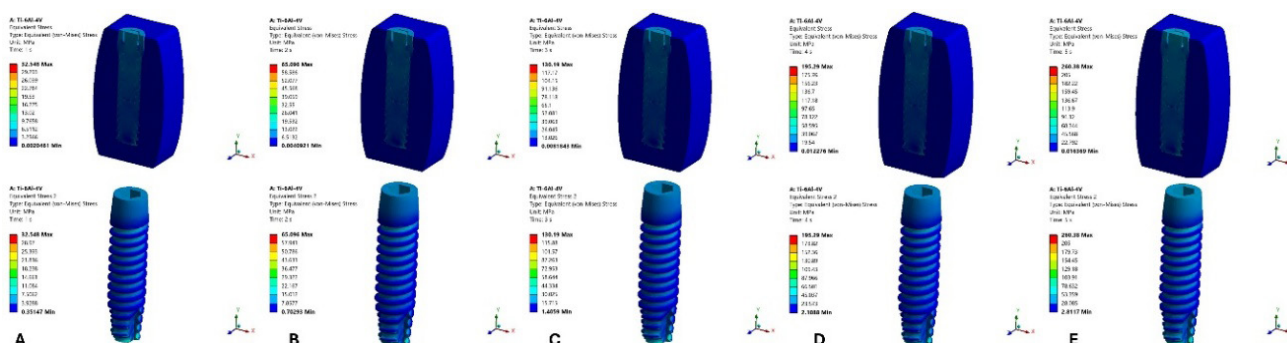


Figure 5. Stress distribution of axial load at 0 degrees in Ti-6Al-4V implant: A) 50 N; B) 100N; C) 200N; D) 300N; E) 400N.

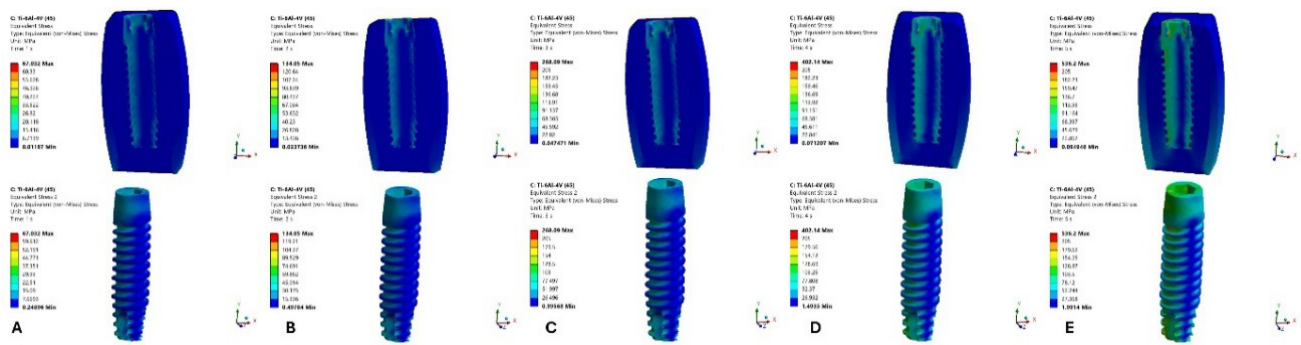


Figure 6. Stress distribution of oblique load at 45 degrees in Ti-6Al-4V implant: A) 50 N; B) 100N; C) 200N; D) 300N; E) 400N.

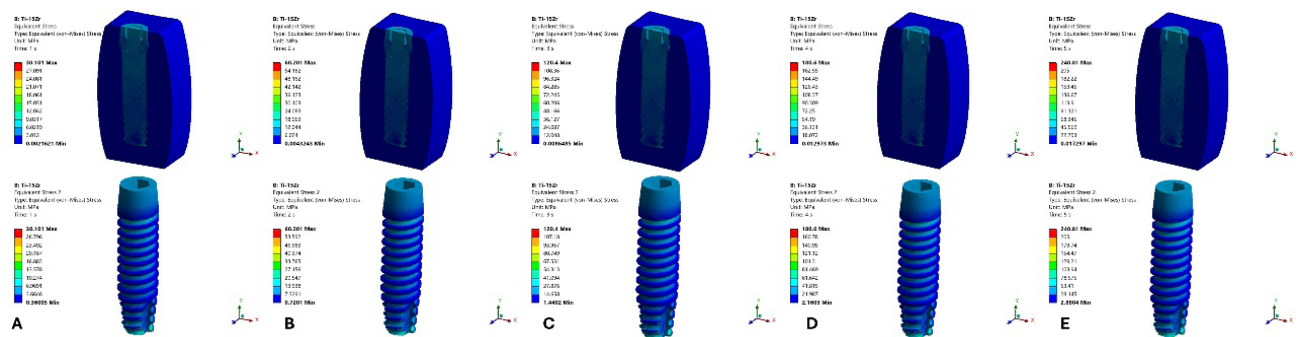


Figure 7. Stress distribution of axial load at 0 degrees in Ti-15Zr implant: A) 50 N; B) 100N; C) 200N; D) 300N; E) 400N.

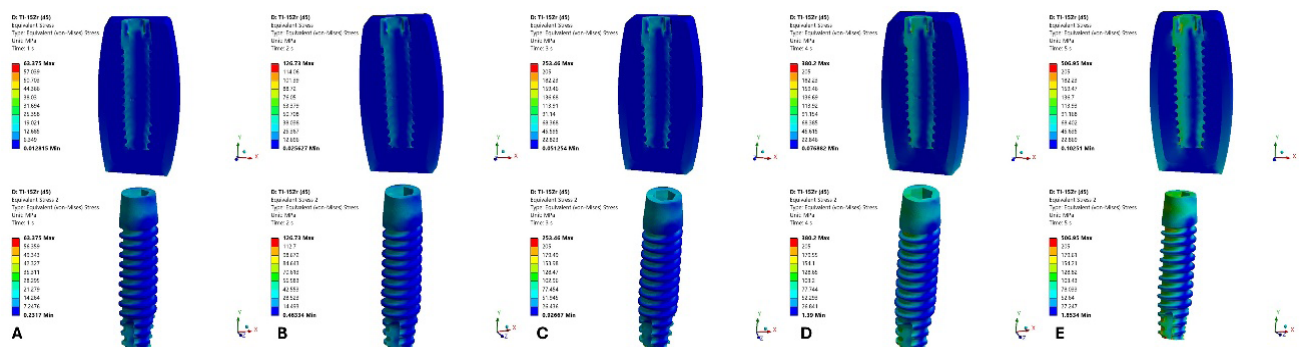


Figure 8. Stress distribution of parafunctional load at 45 degrees in Ti-15Zr implant: A) 50 N; B) 100N; C) 200N; D) 300N; E) 400N.

At the same time, Roxolid-type (Ti-15Zr) reached a peak of around 240.81 MPa, exhibiting a marked stress concentration at the cervical region and the implant-bone junction (Figures 5, 7 and 9).

When oblique loading at 45° was applied, stress patterns changed notably. Titanium alloy Grade 5 subjected to a 50 N up to 400 N oblique parafunctional force registered a bit higher than twice the stress values (67.03 MPa and 536.2 MPa, respectively); with stress localized at the buccal crest and cervical bone (Figure 6). Roxolid-

type implant (Ti-15Zr) exhibited similar behavior under the same parafunctional masticatory conditions, with stress values rising from 63.38 MPa (50 N) to nearly 507 MPa (400 N), the latter remaining clinically safe at yield strength thresholds and indicating a potential protection ability for material fracture. These observations were visually confirmed in stress contour plots, where titanium showed a gradual stress gradient with wider diffusion. At the same time, Roxolid (Ti-15Zr) displayed sharply defined peak stress zones at the implant shoulder (Figures 6, 8 and 9).

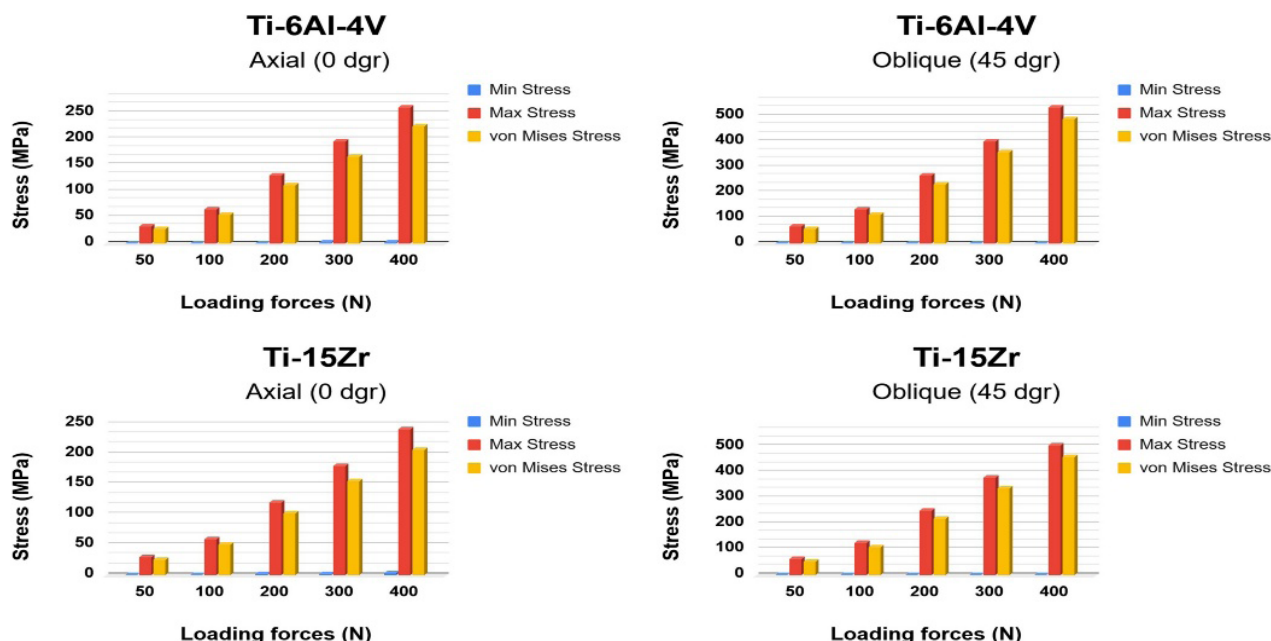


Figure 9. The principal stresses and von Mises values of both one-piece implant types (Ti-6Al-4V and Ti-15Zr) under axial and oblique loading, physiological and parafunctional forces.

The evolution of stress across varying load magnitudes is visually depicted in figure 10. This chart illustrates a linear increase in stress within titanium alloy, which remains within the mechanical safety limits even under severe oblique loading conditions.

On the other hand, Roxolid-based (Ti-15Zr) implants showed an exponential stress response, particularly within the 300–400 N range at 45° angulation, but remaining in the safety zone of the material's vulnerability to fracture (Figure 10). Of particular significance, the steep slope observed in the Ti-15Zr-based implant (45°) curve corroborates biomechanical stability, aligning with earlier mechanical and in vivo investigations that reported fractures in posterior applications [36–41].

When oblique loading at 45° was applied, stress patterns changed notably. Titanium alloy subjected to a 50 N up to 400 N parafunctional force registered a bit higher than twice the stress values (67.03 MPa and 536.2 MPa, respectively); with stress localized at the buccal crest and cervical bone (Figure 6). Roxolid-type implant (Ti-15Zr) exhibited similar behaviour under the same oblique masticatory loading conditions, with stress values rising from 63.38 MPa (50 N) to nearly 507 MPa (400 N), the latter remaining clinically safe at yield strength thresholds and indicating a potential protection ability for material fracture. These observations were visually confirmed in stress contour plots, where titanium showed a gradual stress gradient with wider diffusion. At the same time,

Roxolid-based (Ti-15Zr) displayed sharply defined peak stress zones at the implant shoulder (Figures 6, 8 and 9).

The evolution of stress across varying load magnitudes is visually depicted in figure 10. This chart illustrates a linear increase in stress within titanium alloy, which remains within the mechanical safety limits even under severe oblique loading conditions. On the other hand, Ti-15Zr implants showed an exponential stress response, particularly within the 300–400 N range at 45° but remaining in the safety zone of the material's vulnerability to fracture (Figure 10). Of particular significance, the steep slope observed in the Ti-15Zr (45°) curve corroborates biomechanical stability, aligning with earlier mechanical and in vivo investigations that reported fractures in posterior applications [36–41].

Overall, titanium implants exhibited a resilient stress distribution pattern, with a mechanical response consistent with prior studies by Geng et al. [27] and Himmlova et al. [13], which supports their reliability in load-bearing regions. In contrast, Ti-15Zr's response revealed a similar stress accumulation under parafunctional oblique loads, correlating with fracture-prone regions observed clinically in posterior molar zones [40]. These results underscore the importance of load direction and magnitude in the clinical selection of implant material, and they highlight the Ti-15Zr-based alloy's possibility to withstand complex masticatory forces.

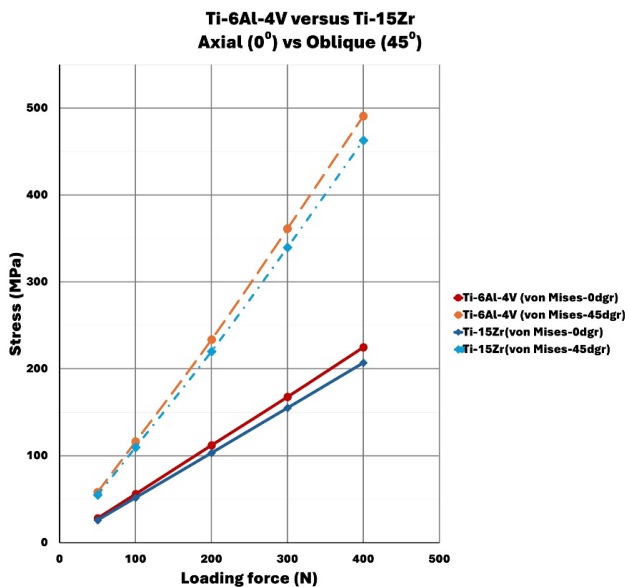


Figure 10. Changes in von Mises stress values for both implant types (Ti-6Al-4V and Ti-15Zr) under axial and oblique loading forces.

Discussion

Occlusion plays an essential role in the stability and osseointegration of dental implants and dental restorations in general [22-26]. Starting from the site of implantation (anterior or posterior), the type of bone (cortical or trabecular), the type of implant (Ti-based, Ti-15Zr-based, Ti-15Zr-Mo-based, alloys etc), its length (long, short), tissue level implantation, or not, convergent neck or not, the general health of the patient, may interfere with the long-term ability of the dental implants to perform and restore the dental tissues functionality [2,4-6,8,11,12,14-19,29-34,36,38,40-46].

The findings of this study show similar mechanical behaviour values between titanium-based alloy and Roxolid-(Ti-15Zr)-based tissue-level convergent collar dental implants under simulated masticatory forces, confirming and expanding on observations reported in recent literature [40-46]. Finite Element Method (FEM) demonstrated that titanium implants distribute occlusal forces evenly and support higher peak von Mises stress values, even under oblique loads. Conversely, Roxolid (Ti-15Zr)-based implants exhibited similar stress concentrations, especially around the implant neck and prosthetic shoulder, under 45° loading (Figure 10). These results align with other literature reports [1,2,5,6,40-46]. Based on these findings, we reject both the H1 and H2 hypotheses.

Moreover, our results are consistent with earlier FEA studies, such as those by Geng et al. [27] and Himmlova et al. [13], which emphasized that material properties, particularly elastic modulus and Poisson's ratio, significantly affect the transfer of stresses from the implant

to the surrounding bone. Titanium alloy (Ti-6Al-4V) has a high stiffness value (110 GPa), which leads to higher stress. In contrast, the Roxolid-type alloy's (Ti-15Zr) stiffness (103.7GPa) results in lower stress peaks under similar conditions, which is consistent with the current simulation.

In their study, Correa et al [41] found the value of YTS (yield tensile strength) for Ti-15Zr-based alloy to be around 555±95MPa. In our study results, the maximum von Mises value was 240.81 MPa (axial load) and 506.95 MPa (oblique load). This indicates that this type of implant alloy material and its design (supracrestal implant with a convergent neck) exhibits favourable mechanical behaviour, remaining predominantly in the elastic zone, especially when paraxial forces are applied. Our findings also correlate strongly with other in vitro fatigue testing and clinical reports [5,6,21,22,31,34,35,45-50]. Moreover, we chose to use the tissue-level and convergent neck design for our experimental implants based on other studies that demonstrated their clinical reliability in terms of implant design [30,42,49,51].

On one side, Canullo et al [30] showed that tissue-level convergent neck implants performed well in the anterior region, and Ioannidis et al [43] showed that Ti-15Zr-based alloy implant performed well in the frontal low-load zones and also in the premolar area when using a 3.3 mm diameter implant; on the other side, in our study, we found a good mechanical performance for an implant tested in the mandibular molar region, with a 3.8 mm diameter, which is also consistent with other studies [33,36,40].

It is well known that occlusal forces and cyclic loading may cause the implant materials to behave differently along with oral soft and hard tissues [23-26,44-46]. In the given conditions, to better understand what may happen with the implant materials in the lateral zone, we subjected them to a simulation of physiological and parafunctional masticatory forces; thus, we used axial (0 degrees) and oblique (45 degrees) forces with a range of increasing forces (50N, 100N, 200N, 300N, 400N). The higher values of the masticatory forces (300N and 400N) were observed during grinding or clenching teeth [23-26,52]; thus, we used them to observe the mechanical behaviour of our tested implants.

Brizuela et al [53] demonstrated that a low modulus of elasticity can promote better osseointegration of alloy-based materials used in dental implantology. In our case, the Roxolid-type Ti-15Zr implant with the attributed tissue-level with a convergent collar, remained within the elastic domain even under parafunctional masticatory forces, when compared to the Ti-6Al-4V implant with the same attributed design. Therefore, we believe that the design type and low von Mises stress values contribute to Roxolid-type implants facilitating osseointegration.

The mechanical findings are further interpreted in the light of recent histological, microbiological, and clinical data, offering a comprehensive perspective on

the indications and limitations of each material in modern implantology. Thus, histological and immunohistochemical studies have demonstrated improved epithelial adhesion, greater collagen fibre orientation, and reduced expression of inflammatory markers around Roxolid-type (Ti-15Zr) surfaces, which may support long-term peri-implant health [11,12]. Additionally, Roxolid (Ti-15Zr) implants are a valuable solution for patients with a confirmed titanium allergy or those with systemic inflammatory conditions that are aggravated by metal ions [19].

From a biological perspective, Roxolid-type (Ti-15Zr) implants continue to demonstrate notable advantages. Numerous studies, including those by Scarano et al. [10], Kniha et al. [11], and Depprich et al [12], have confirmed that bacterial adhesion to Roxolid-type (Ti-15Zr) is lower than to titanium, which may translate to reduced rates of mucositis and peri-implantitis in clinical practice. Furthermore, soft tissue studies indicate that Roxolid (Ti-15Zr) promotes more favourable fibroblast adhesion and collagen fibre orientation, which can help maintain long-term mucosal sealing and aesthetic outcomes [11,12,20].

These soft tissue advantages, however, must be weighed against the biomechanical risks highlighted in this study and others [38-46]. While titanium has been associated with increased plaque accumulation and corrosion in some instances, it remains the most thoroughly validated material in implant dentistry, with over four decades of clinical data supporting its use in both anterior and posterior regions [3].

Despite growing clinical acceptance, Roxolid-type (Ti-15Zr) implant systems have not yet achieved the same level of scientific and regulatory validation as titanium-based systems. Most Roxolid (Ti-15Zr)-based implant studies are limited by short follow-up periods (<5 years), small sample sizes, and heterogeneity in implant geometry and surface topography [20,21].

Thus, clinically, the decision to use Roxolid-type (Ti-15Zr) or titanium-based alloy should be guided not only by aesthetic requirements or material preference, but also by a comprehensive understanding of the biomechanical environment. For patients with high bite forces, posterior molar restorations, or parafunctional habits, titanium remains the material of choice. On the other hand, Roxolid-based alloy (Ti-15Zr) may be favoured in thin biotypes, aesthetic zones, or in patients with metal allergies or a history of soft tissue sensitivity [41-47].

Nevertheless, in the past decade, new studies have emerged that aim to combine different metallic or non-metallic elements with titanium for improved mechanical or biological outcomes in modern implantology [53-56].

Despite its findings, this study has some limitations that need to be underlined:

- First, the analysis was based on static loading conditions, which do not replicate the complex, dynamic, and cyclic nature of actual mastication. In clinical scenarios, implants experience repeated micro-movements

and fatigue over thousands of cycles, which could affect long-term mechanical behavior differently than static simulations predict.

- Secondly, the model assumed that all components, including bone, have homogeneous, isotropic, and linearly elastic material properties. In reality, bone shows anisotropic and viscoelastic behavior that might influence load transfer, especially at the bone-implant interface.

- Thirdly, only one implant geometry (tissue-level with convergent neck design) was examined. While this standardization facilitates direct material comparison, it does not consider variations in implant macro-designs (e.g., tapered vs. parallel walls, thread pitch) that could notably affect stress distribution.

- Fourth, no prosthetic components (such as crowns or abutments) were modeled, and the load was applied directly on the implant platform. While this simplifies the analysis and highlights implant body mechanics, it overlooks the potential effects of prosthetic misfit, occlusal surface design, or cement layer properties.

- Finally, the lack of biological factors, such as bone remodeling, immune response, and healing dynamics, limits the interpretation of results to only mechanical behaviour.

- Real-world outcomes rely on a complex interaction between biomechanics and biology, which cannot be fully captured by FEA alone.

Future research should incorporate dynamic load simulations, fatigue testing, anisotropic bone modelling, and expanded implant geometries to generate more clinically relevant conclusions. Despite these limitations, the current model provides a solid and controlled comparison between Roxolid-type (Ti-15Zr) and titanium-based implants, emphasizing key differences that are important for clinical decision-making.

Conclusions

Within the limits of this experimental study, we may conclude the following:

1. Roxolid-type (Ti-15Zr) implants exhibit similar biomechanical performance to titanium-based materials when subjected to increasing masticatory forces under both axial and oblique loads.

2. Finite element analysis revealed that Ti-15Zr-based implants consistently maintained lower von Mises stress values and more favourable stress distribution across the implant and surrounding bone, even at the maximum applied load of 400 N at a 45° inclination.

3. Ti-6Al-4V implants showed significantly higher peak stress concentrations, especially at the implant shoulder and crestal bone interface.

4. Roxolid-type (Ti-15Zr) alloy remains a valuable implant material in specific clinical situations. However, its use should be limited to carefully selected cases with controlled occlusion and minimal lateral forces.

5. Under the FEA simulation, the tissue-level convergent collar design demonstrated good mechanical behavior for both tested alloy materials.

Acknowledgements

The authors would like to thank the Department of Mechanical Engineering, Materials Resistance, from the Technical University Cluj-Napoca.

References

- Gottlow J, Dard M, Kjellson F, Obrecht M, Sennerby L. Evaluation of a new titanium-zirconium dental implant: a biomechanical and histological comparative study in the mini pig. *Clin Implant Dent Relat Res*. 2012;14:538-545.
- Haimov E, Sarikov R, Haimov H, Juodzbalsys G. Differences in Titanium, Titanium-Zirconium, Zirconia Implants Treatment Outcomes: a Systematic Literature Review and Meta-Analysis. *J Oral Maxillofac Res*. 2023;14:e1.
- Steinemann SG. Titanium--the material of choice? *Periodontol* 2000. 1998;17:7-21.
- Nakagawa M, Matsuya S, Udoh K. Corrosion behavior of pure titanium and titanium alloys in fluoride-containing solutions. *Dent Mater J*. 2001;20:305-314.
- Sotova C, Yanushevich O, Kriehli N, Grigoriev S, Evdokimov V, Kramar O et al. Dental Implants: Modern Materials and Methods of Their Surface Modification. *Materials (Basel)*. 2023;16:7383.
- Anchieta RB, Baldassarri M, Guastaldi F, Tovar N, Janal MN, Gottlow J, et al. Mechanical property assessment of bone healing around a titanium-zirconium alloy dental implant. *Clin Implant Dent Relat Res*. 2014;16:913-919.
- Sivaraman K, Chopra A, Narayan AI, Balakrishnan D. Is zirconia a viable alternative to titanium for oral implant? A critical review. *J Prosthodont Res*. 2018;62:121-133.
- Duan C, Ye L, Zhang M, Yang L, Li C, Pan J et al. Clinical performance of zirconium implants compared to titanium implants: a systematic review and meta-analysis of randomized controlled trials. *PeerJ*. 2023;11:e15010.
- Chang SH, Li ZY. Effect of oxidation at an elevated temperature on the evolution of phases, microstructure, and properties of the oxide films formed on the surface of TiZr. *Sci Rep*. 2023;13:5126.
- Scarano A, Piattelli M, Caputi S, Favero GA, Piattelli A. Bacterial adhesion on commercially pure titanium and zirconium oxide disks: an in vivo human study. *J Periodontol*. 2004;75:292-296.
- Kniha K, Heussen N, Modabber A, Hölzle F, Möhlhenrich SC. The effect of zirconia and titanium surfaces on biofilm formation and on host-derived immunological parameters. *Int J Oral Maxillofac Surg*. 2021;50:1361-1374.
- Depprich R, Zipprich H, Ommerborn M, Mahn E, Lammers L, Handschel J et al. Osseointegration of zirconia implants: an SEM observation of the bone-implant interface. *Head Face Med*. 2008;4:25.
- Himmlová L, Dostálová T, Kácovský A, Konvicková S. Influence of implant length and diameter on stress distribution: a finite element analysis. *J Prosthet Dent*. 2004;91:20-25.
- Liu X, Chen S, Tsoi JKH, Matinlinna JP. Binary titanium alloys as dental implant materials-a review. *Regen Biomater*. 2017;4:315-323.
- Comisso I, Arias-Herrera S, Gupta S. Zirconium dioxide implants as an alternative to titanium: A systematic review. *J Clin Exp Dent*. 2021;13:e511-e519.
- Barlattani A Jr, Martelli M, Ceruso FM, Gargari M, Ottria L. Convergent implant transmucosal collar and healing abutment: aesthetics influence on soft tissues. A clinical study. *J Biol Regul Homeost Agents*. 2020;34:63-69.
- Sadid-Zadeh R, Willis J, Forgo G, Haraszthy V. Comparative Analysis of Biofilm Formation on Materials Used for the Fabrication of Implant-Supported Prostheses. *Braz Dent J*. 2020;31:380-384.
- Fretwurst T, Müller J, Larsson L, Bronsert P, Hazard D, Castilho RM et al. Immunohistological composition of peri-implantitis affected tissue around ceramic implants-A pilot study. *J Periodontol*. 2021;92:571-579.
- Poli PP, de Miranda FV, Polo TOB, Santiago Júnior JF, Lima Neto TJ, Rios BR et al. Titanium Allergy Caused by Dental Implants: A Systematic Literature Review and Case Report. *Materials (Basel)*. 2021;14:5239.
- Jiang T, Wu H, Fu S, Chen X, Liu P. Recent progress in manufacturing technology, element addition, and surface modification of TiZr materials in dental implants. *Journal of Materials Research and Technology* 2025;37:5491-5513.
- Cruz MB, Silva N, Marques JF, Mata A, Silva FS, Caramês J. Biomimetic Implant Surfaces and Their Role in Biological Integration-A Concise Review. *Biomimetics (Basel)*. 2022;7:74.
- Aldowish AF, Alsubaie MN, Alabdulrazzaq SS, Alsaykhan DB, Alamri AK, Alhatem LM et al. Occlusion and Its Role in the Long-Term Success of Dental Restorations: A Literature Review. *Cureus*. 2024;16:e73195.
- Martinez-Mondragon M, Urriolagoitia-Sosa G, Romero-Ángeles B, García-Laguna MA, Laguna-Canales AS, Pérez-Partida JC et al. Biomechanical Fatigue Behavior of a Dental Implant Due to Chewing Forces: A Finite Element Analysis. *Materials (Basel)*. 2024;17:1669.
- Shala K, Tmava-Dragusha A, Dula L, Pustina-Krasniqi T, Bicaj T, Ahmedi E et al. Evaluation of Maximum Bite Force in Patients with Complete Dentures. *Open Access Maced J Med Sci*. 2018;6:559-563.
- Hernández-Vázquez RA, Romero-Ángeles B, Urriolagoitia-Sosa G, Vázquez-Feijoo JA, Vázquez-López AJ, Urriolagoitia-Calderón G. Numerical Analysis of Masticatory Forces on a Lower First Molar considering the Contact between Dental Tissues. *Appl Bionics Biomech*. 2018;2018:4196343.
- Poli O, Manzon L, Niglio T, Ettore E, Voza I. Masticatory Force in Relation with Age in Subjects with Full Permanent Dentition: A Cross-Sectional Study. *Healthcare (Basel)*. 2021;9:700.
- Geng JP, Tan KB, Liu GR. Application of finite element

- analysis in implant dentistry: a review of the literature. *J Prosthet Dent.* 2001;85:585-598.
28. Cruz RS, Lemos CAA, de Batista VES, Yogui FC, Oliveira HFF, Verri FR. Narrow-diameter implants versus regular-diameter implants for rehabilitation of the anterior region: a systematic review and meta-analysis. *Int J Oral Maxillofac Surg.* 2021;50:674-682.
29. Anitua E, Larrazabal Saez de Ibarra N, Morales Martín I, Saracho Rotaache L. Influence of Dental Implant Diameter and Bone Quality on the Biomechanics of Single-Crown Restoration. A Finite Element Analysis. *Dent J (Basel).* 2021;9:103.
30. Canullo L, Menini M, Covani U, Pesce P. Clinical outcomes of using a prosthetic protocol to rehabilitate tissue-level implants with a convergent collar in the esthetic zone: A 3-year prospective study. *J Prosthet Dent.* 2020;123:246-251.
31. Gao Y, He X, Xu W, Deng Y, Xia Z, Chen J, He Y. Three-dimensional finite element analysis of the biomechanical properties of different material implants for replacing missing teeth. *Odontology.* 2025;113:80-88.
32. Velasco-Ortega E, Flichy-Fernández A, Punset M, Jiménez-Guerra A, Manero JM, Gil J. Fracture and Fatigue of Titanium Narrow Dental Implants: New Trends in Order to Improve the Mechanical Response. *Materials (Basel).* 2019;12:3728.
33. Yang F, Liu D, Yin W, Yuan C, Hu Y, Xu J, Yang Y, Tang J, Chen J. Three-dimensional finite element analysis of the biomechanical behaviour of different dental implants under immediate loading during three masticatory cycles. *Heliyon.* 2024;10:e32616.
34. Brizuela-Velasco A, Pérez-Pevida E, Jiménez-Garrudo A, Gil-Mur FJ, Manero JM, Punset-Fuste M et al. Mechanical Characterisation and Biomechanical and Biological Behaviours of Ti-Zr Binary-Alloy Dental Implants. *Biomed Res Int.* 2017;2017:2785863.
35. Chatterjee E, Nasha A, Mustafa M, Chinthalapudi SL, Padavala S, Lakshmpuram AK et al. The Impact of Implant Angulation on the Stress Distribution and Survival Rate of Implant-Supported Fixed Dental Prostheses: A Retrospective Study. *Cureus.* 2023;15:e47892.
36. Hanes B, Feitosa S, Phasuk K, Levon JA, Morton D, Lin WS. Fracture Resistance Behaviors of Titanium-Zirconium and Zirconia Implants. *J Prosthodont.* 2022;31:441-446.
37. Medvedev AE, Molotnikov A, Lapovok R, Zeller R, Berner S, Habersetzer P et al. Microstructure and mechanical properties of Ti-15Zr alloy used as dental implant material. *J Mech Behav Biomed Mater.* 2016;62:384-398.
38. Pérez RA, Gargallo J, Altuna P, Herrero-Climent M, Gil FJ. Fatigue of Narrow Dental Implants: Influence of the Hardening Method. *Materials (Basel).* 2020;13:1429.
39. Zhao Q, Ueno T, Wakabayashi N. A review in titanium-zirconium binary alloy for use in dental implants: Is there an ideal Ti-Zr composing ratio? *Jpn Dent Sci Rev.* 2023;59:28-37.
40. Valente NA, Wu M, Toti P, Derchi G, Barone A. Impact of Concave/Convergent vs Parallel/ Divergent Implant Transmucosal Profiles on Hard and Soft Peri-implant Tissues: A Systematic Review with Meta-Analyses. *Int J Prosthodont.* 2020;33:553-564.
41. Correa DRN, Rocha LA, Donato TAG, Sousa KSJ, Grandini CR, Afonso CRM, et al. On the mechanical biocompatibility of Ti-15Zr-based alloys for potential use as load-bearing implants. *J Mater Res Tech.* 2020;9:1241-1250.
42. Parize HN, Bohner LOL, Gama LT, Porporatti AL, Mezzomo LAM, Martin WC et al. Narrow-diameter implants in the anterior region: A meta-analysis. *Int J Oral Maxillofac Implants.* 2019;34:1347-1358.
43. Ioannidis A, Gallucci GO, Jung RE, Borzangy S, Hämmerle CH, Benic GI. Titanium-zirconium narrow-diameter versus titanium regular-diameter implants for anterior and premolar single crowns: 3-year results of a randomized controlled clinical study. *J Clin Periodontol.* 2015;42:1060-1070.
44. Fathi A, Borhani S, Salehi S, Mosharrar R, Atash R. Effect of Thermodynamic Cyclic Loading on Screw Loosening of Tightened Versus New Abutment Screw in Bone Level and Tissue Level Implants in DIO Implant Company (In-Vitro Study). *Clin Exp Dent Res.* 2025;11:e70162.
45. Borges Radaelli MT, Idogava HT, Spazzin AO, Noritomi PY, Boscato N. Parafunctional loading and occlusal device on stress distribution around implants: A 3D finite element analysis. *J Prosthet Dent.* 2018;120:565-572.
46. Silva LS, Verri FR, Lemos CAA, Martins CM, Pellizzer EP, de Souza Batista VE. Biomechanical effect of an occlusal device for patients with an implant-supported fixed dental prosthesis under parafunctional loading: A 3D finite element analysis. *J Prosthet Dent.* 2021 Aug;126:223.e1-223.e8.
47. Xiao W, Chen Y, Chu C, Dard MM, Man Y. Influence of implant location on titanium-zirconium alloy narrow-diameter implants: A 1-year prospective study in smoking and nonsmoking populations. *J Prosthet Dent.* 2022;128:159-166.
48. Costa Castillo M, Laguna Martos M, Marco Pitarch R, García Selva M, Del Cid Rodríguez S, Fons-Badal C et al. Analysis of Peri-Implant Bone Loss with a Convergent Transmucosal Morphology: Retrospective Clinical Study. *Int J Environ Res Public Health.* 2022;19:3443.
49. Ionescu A, Dodi A, Panagopoulos V, Nicolescu MI, Mihai AT, Tanase G, Vlasceanu D. Biomechanical consequences of dental implants inserted in augmented alveolar ridges – a comparative study between tissue-level and bone-level implants: finite elements analysis. *Rom J Oral Rehabilitation* 2019;11:69-75.
50. Ghasemi E, Fathi A, Jahangiri S, Farahmand S. Evaluation of the effect of different angles and positions of implants on stress distribution in bone and prosthetic structures in reconstruction of complete maxillary arch with all-on-four concept: 3d finite element analysis. *Rom J Oral Rehabilitation* 2025;17:73-92.
51. Müller F, Al-Nawas B, Storelli S, Quirynen M, Hicklin S, Castro-Laza J et al. Roxolid Study Group. Small-diameter titanium grade IV and titanium-zirconium implants in edentulous mandibles: five-year results from a double-blind, randomized controlled trial. *BMC Oral Health.* 2015;15:123.
52. Yadav K, Kumar S, Aggarwal R, Kaur I, Goyal A, Sharma R et al. Finite Element Analysis of Platform Switching Effects on Stress Distribution in Posterior Implants Placed in Different Bone Types Under Axial and Oblique Loading Conditions.

Cureus. 2025;17:e86821.

53. Brizuela A, Herrero-Climent M, Rios-Carrasco E, Rios-Santos JV, Pérez RA, Manero JM et al. Influence of the Elastic Modulus on the Osseointegration of Dental Implants. *Materials*. 2019; 12:980.
54. Zapata JM, Leal E, Hunter R, de Souza RF, Borie E. Biomechanical Behavior of Narrow Dental Implants Made with Aluminum- and Vanadium-Free Alloys: A Finite Element Analysis. *Materials*. 2022; 15:8903.
55. Lourenço ML, Cardoso GC, Sousa KDSJ, Donato TAG, Pontes FML, Grandini CR. Development of novel Ti-Mo-Mn alloys for biomedical applications. *Sci Rep*. 2020;10:6298.
56. Calazans Neto JV, Celles CAS, de Andrade CSAF, Afonso CRM, Nagay BE, Barão VAR. Recent Advances and Prospects in β -type Titanium Alloys for Dental Implants Applications. *ACS Biomater Sci Eng*. 2024;10:6029-6060.